


Featured PT Tip Brief

Spot Trending Data Points That Suggest a Possible **“Not Acceptable”**

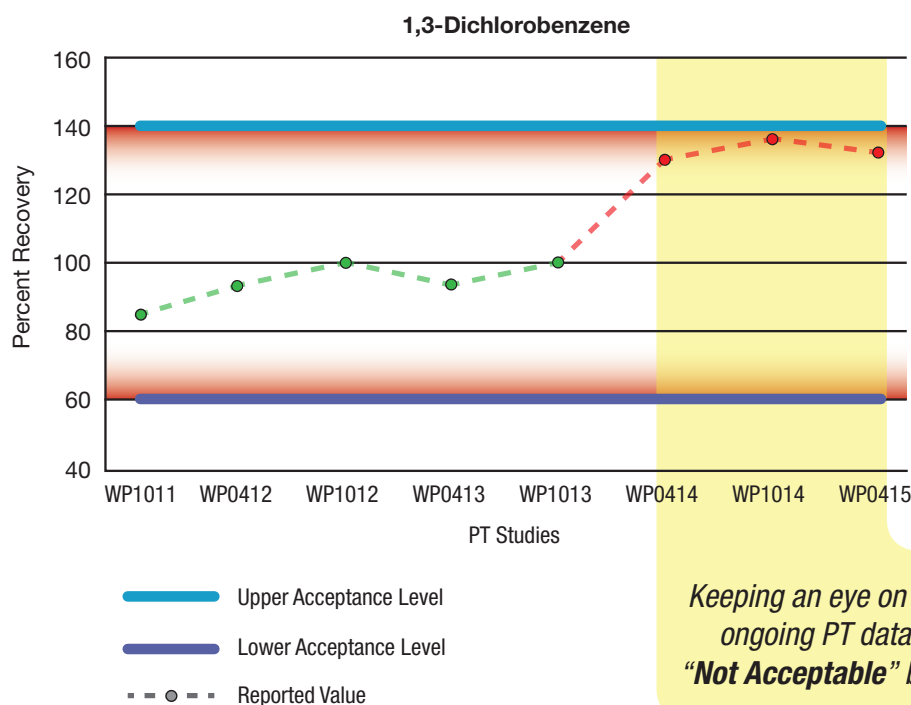

*Keeping an eye on your laboratory's ongoing PT data can prevent a **“Not Acceptable”** before it happens!*

CATEGORY:

- ☒ PT Analytics
- ☐ Corrective Action
- ☐ Ordering
- ☐ Data Entry
- ☐ Technical

PT data trending towards an out of range bias may signal a possible systemic error within the

- Method
- Instrumentation
- Calibration
- Reference materials

Use PT Manage's Custom Report Generator




PT ManageTM
Analytics & Reporting Software

Phenova's PT management software allows you to customize reports that illustrate your laboratory's progress for specific PT studies across a designated time period using the Custom Report Generator.


Online Demo

Learn How to Use Our Custom Report Generator

Visit www.phenova.com/CustomReports

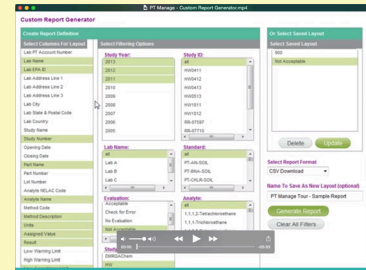

3 steps to identify a potential "Not Acceptable" using the Custom Report Generator

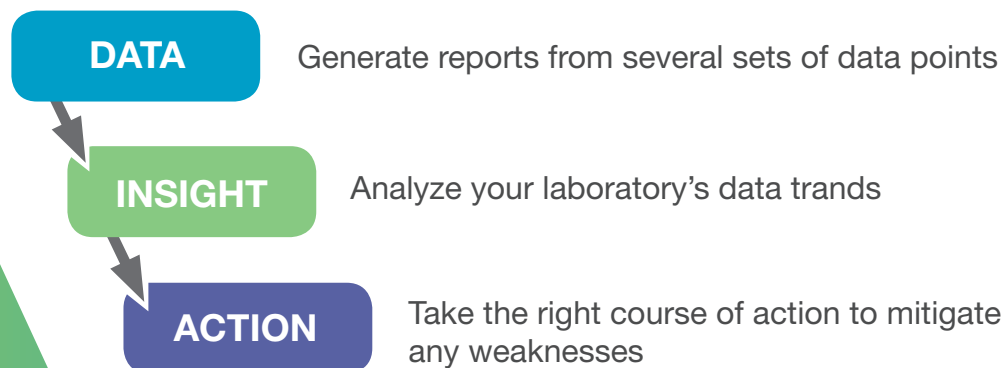

For More Information on PT Manage Visit
www.Phenova.com/PTManage

Terms and Conditions
Subject to Phenova Standard Terms and Conditions, which may be viewed at www.phenova.com/TermsAndConditions.

Trademarks
Phenova is a registered trademark and PT Manage is a trademark of Phenova, Inc., an affiliate of Phenomenex, Inc.
© 2015 Phenova, Inc. All rights reserved.

Let Us Show You How to Review Your Laboratory's PT Data Trends

Contact Us | 1-866-942-2978 | info@phenova.com